

Quick Start Guide:

SCIO on Pulsar

Safety Info	2
1. Pulsar Software Installation	2
2. Plug and Play: Hardware Setup	2
3. Your First Session	3
3.1 Demographics	3
3.2 Calibration	5
3.2.1 In-Harness Patients	5
3.2.2 Distance / Subspace Patients	6
3.2.3 Adjusting Calibration If Necessary	6
3.3 Home Use Therapies	7
3.4 Timed Therapies	7
3.5 Closing A Session	10
3.5.1 Release Snags or 'Hooks'	10
3.5.2 Balancing Chakras	11
3.5.2 Strengthening the Aura	11
4. Don't Damage Your Equipment	12
4.1 Make Your Electrodes Last Longer	12
4.2 Cleaning the SCIO	12
4.3 Aeroplanes, X-Rays & Travel	13
5. Repairs and Replacements	13

Quantum Medical S.R.L., Str Randunelelor 19, Satu Mare, Romania, 440049

Technical Support: +40 744 258 668 | info@quantum-medical.eu

The National Centre for ElectroMagnetic Therapies C.I.C., Registered in England & Wales under Company Number 11486072

Sales and Training: +44 7394 870 156 | admin@ncet.co.uk

Safety Info

Don't work on a patient who is wearing a pace-maker.

A pace-maker is an electrical, mechanical apparatus to help control the heartbeat. The SCIO device may cause the pace-maker to be reset or need resetting.

Put a power cord or electrical surge protector between the computer and the main wall socket.

A surge protector is an extension cord standing in between the main wall socket and the computer, which is directly connected to the SCIO device. It is best to use an electrical surge protector in case of a lightning strike or other electrical malfunction coming from the main building's power source.

The SCIO device has electrical safety measures built in, namely, to convert Alternating Current (AC) which is deadly for living creatures into Direct Current (DC) and to store the incoming electricity and regulate its output.

1. Pulsar Software Installation

Download and run the Pulsar .exe file found at the bottom of this page:

<https://ncet.co.uk/pulsar-scio>

Make sure you've signed up to pay monthly for Pulsar, and that we've entered your SCIO serial number into our database for activation.

2. Hardware Setup

(1) Plug the SCIO into the computer in exactly this way:

One end of the USB-to-USB cable first plugs into the SCIO box. The other end of the USB cable goes into your computer directly.

Switch the SCIO box on.

(2) Next, start the software Pulsar.

When the launch process has loaded 25%, it will stop and ask you to select a

Quantum Medical S.R.L., Str Randunelelor 19, Satu Mare, Romania, 440049 Technical Support: +40 744 258 668 info@quantum-medical.eu The National Centre for ElectroMagnetic Therapies C.I.C., Registered in England & Wales under Company Number 11486072 Sales and Training: +44 7394 870 156 admin@ncet.co.uk
--

user or create a new user, then click “OK” to continue.

(3) Attach the electrode harnesses:

The HEAD harness with the cable on the patient’s RIGHT side of their body.

Attach the LIMB harness:

RED on the RIGHT wrist

BLUE on the RIGHT ankle

YELLOW on the LEFT wrist

BLACK on the LEFT ankle

The connection is strongest when electroconductive gel is placed on the electrodes then applied directly to the patient’s skin. A less sticky or messy alternative is to use a facial tissue (such as Kleenex) and dampen it thoroughly with either pure distilled water, or a 50/50 mixture of hydrogen peroxide and distilled water.

3. Your First Session

Pulsar stops loading at 25% progress and asks you to select a user and language, then the password screen pops up automatically. Enter:

0210

Hit the “Enter” key or click “OK”.

3.1 Demographics

The yellow Demographics window opens up automatically. Enter new patient information by clicking the button “New Patient” and completing the information. It should be easy enough to figure out.

For in-harness patients, it doesn’t matter so much that you enter in their complete name or time of birth. The date of birth is helpful in calculating Biorhythms, and then mitigating any negative effects from disharmonious Biorhythms / astrological influences so that the session runs more smoothly.

For distance (also called “subspace”) sessions, click on the top navigation menu item “Birth Time and Place” at the top of the panel, and enter the patient’s exact time of birth in 24-hour format as well as latitude and longitude where they were born. Look up this information on Google Maps – see screenshots below.

Demographics

Patient Data **Birth Time and Place** Backup and Restore Demographics Report

Patients

Today is: 2023/03/08 Visit # - 0

Name: Use Gender specific Matrix: ☐

Date of Birth: ☐ Male ☐ Female

☐ Pregnant

Place of Birth:


Country: Inherited Disorder: ☐

Amount of negativity 0-10:

BMI:

Only for distance / subspace clients: Head to <https://maps.google.com> and enter the exact address of their birth, for example the hospital. Grab the latitude and longitude of that location from the URL in Google Maps.

Here’s the latitude, after the location’s name in the URL (the next screenshot is larger and easier to see the exact numbers):

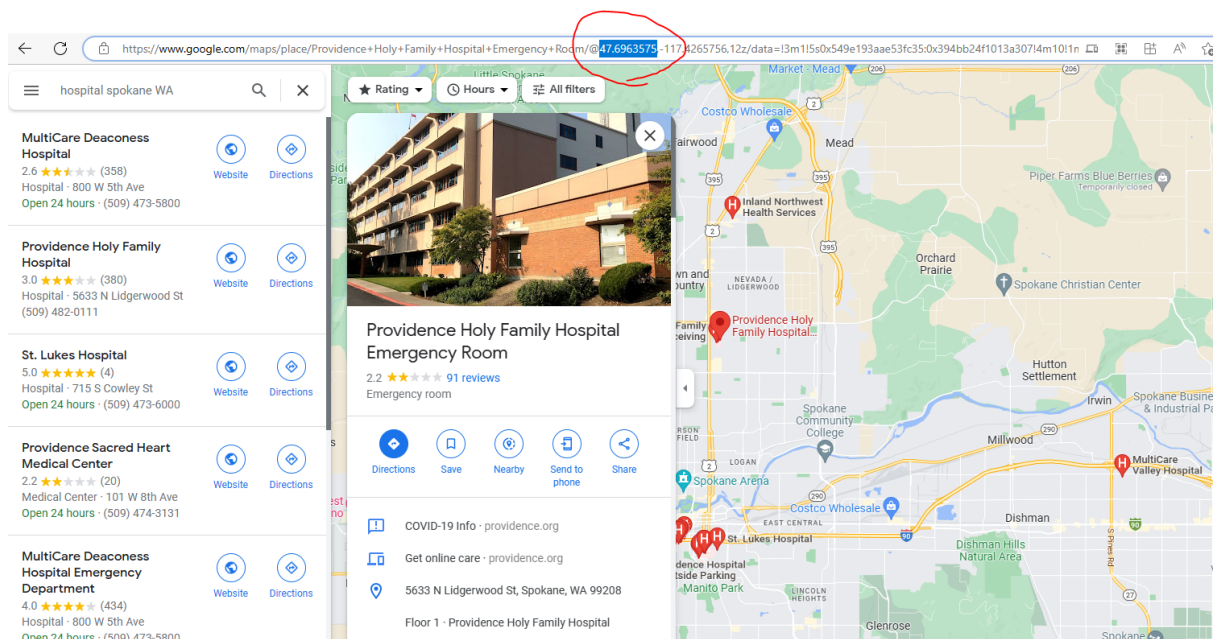


Quantum Medical S.R.L., Str Randunelelor 19, Satu Mare, Romania, 440049

Technical Support: +40 744 258 668 | info@quantum-medical.eu

The National Centre for ElectroMagnetic Therapies C.I.C., Registered in England & Wales under Company Number 11486072

Sales and Training: +44 7394 870 156 | +44 3301330183 | admin@ncet.co.uk

The next screenshot is larger and easier to see the exact numbers:

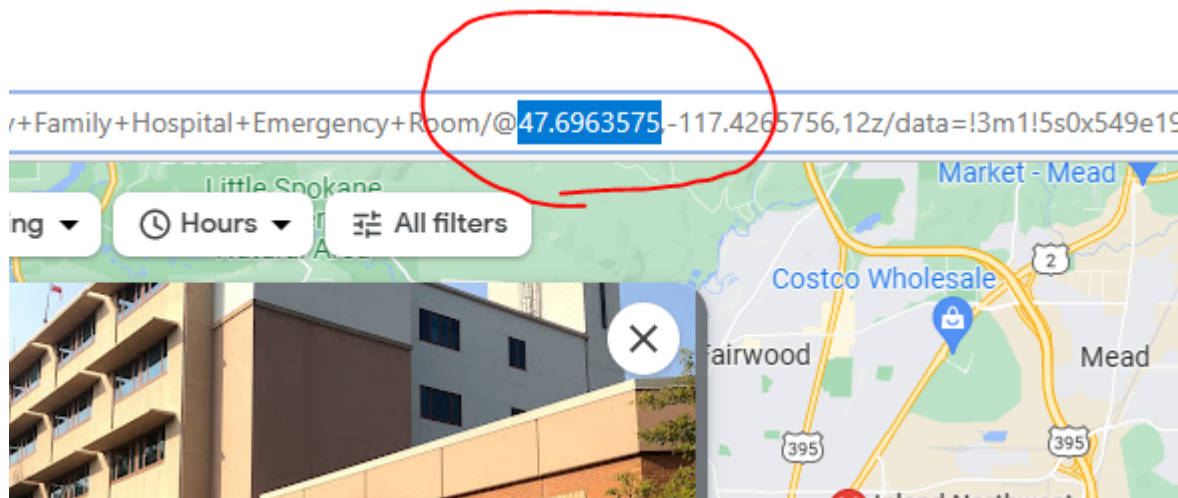

That's the latitude. The next number in that URL after the comma is the longitude. Include the minus sign (-) if there is one (for North and South America, for example) when you copy-paste it.

Skip filling in the SOC information; it just takes up extra time. Hit "Save" and you're done with the demographics.

If you have some questions about any buttons or areas that aren't covered in this very brief Quick Start Guide, then please visit the Quantum Medical Knowledgebase:

<https://support.quantum-medical.eu/post-list/>

3.2 Calibration

After saving the New Patient Information, you return automatically to the main menu page. Click on the button second from the top in the main column, "Calibration".

Click on the button "Computer Risk Field Neutralization" and on the pop-up window click "Show + Tune Harmonics". Next, click the button "Check Room for Geopathic Stress" then follow the instructions or your common sense. If stress is detected, click on the button to clean it.

3.2.1 In-Harness Patients

Have your patient remove jewellery, mobile phones, and any electronic devices that may interfere with the machine's calibration and readings.

Next, click the button “Calibration Program” toward the top right-hand corner of the window.

3.2.2 Distance / Subspace Patients¹


For distance / subspace sessions, you can skip cleaning geo stress from the room and neutralising the computer risk field if you want to save time. It’s only helpful for a more accurate connection, which depends largely upon your own mind / consciousness / focus and purity.

Just click on the button “Virtual All” on the left side of that window, then click on the button “Calibration Program” in the upper right-hand corner.

For in-harness sessions, do not click on “Virtual All” before running Calibration.

3.2.3 Adjusting Calibration If Necessary

After calibration is complete, do not close the pop-up window that says “Calibraiton is complete, would you like to close? Yes / No.” Click and drag that pop-up down so you can see what’s behind it. Look for the calibration accuracy:

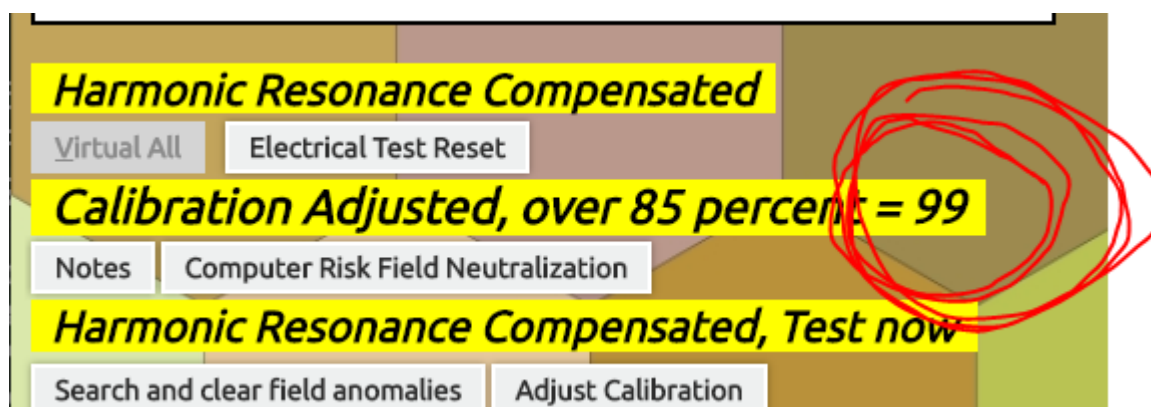

If it is 95% or higher, then close calibration.

If it’s 94% or lower, you want to re-calibrate so that it’s higher. To re-calibrate, click the button “Search and clear field anomalies” then click the button “Adjust Calibration”. Keep clicking “Adjust Calibration” until you get 95% or higher.

More accurate calibration means that the ‘grip’ of the machine on the patient’s body is tighter, so the session will go better.

Close that window and move on to 3.3 and / or 3.4 below.

¹ Usually these folks are called “clients” rather than “patients” in the UK, but do whatever you think regulations in your country allow

3.3 Home Use Therapies

The easiest thing you can do is let the machine run on its AI-guided programmes. Don't worry about doing more complicated things, you can learn them in due course.

From the main menu panel, click on the button "Home Use".

On this window, you can select as many therapies as you'd like. What you see is what you get: General Wellness, Insomnia, etc. – click on the button to select the therapy, set the number of minutes to the right side (at least 10 minutes for each is recommended), then hit "Start" at the bottom.

The minimum duration is 1 minute; the maximum duration is 15 or 25 minutes depending on the therapy. Just try typing in a number of minutes and you'll find out.

Select as many therapies as you'd like. Click "start" – obviously! – at the bottom of the window to start running each therapy one after the other. After each therapy run is complete, you'll see a rectification number on the right side: 85% or higher is ideal and means that therapy run went as well as possible.

You can re-run a therapy selection by waiting until all have completed, then hitting the "Start" button again once all therapies have finished running. To remove a therapy from the 'playlist', click on its button to deselect it.

3.4 Timed Therapies

This is an old, tried-and-true therapy window. Find it from the Main Menu panel in the long column, fourth button from the top, "Therapy". That brings up a busy-looking window. Click on the button toward the bottom: "Timed Therapies, Music and Super-Learning":

Universal Biofeedback Therapy

percent successful 0 %

Report

Test Time Spent

Start

Timer in Min.5 max 0

TIME

Auto Trivector Therapy Suggested

Auto Meridian/ Hyper-Reactants

Spinal Auto VARHOPE

Auto Scalar Mental NLP Interface

Auto Freq Therapy

Auto Trivector

Auto Color Therapy

Activation Type

☐ Activate Tray

☐ Activate Harness

☐ Activate Virtual

☒ Activate All

Text Explaining Rife and Bioresonance

TriVector and Hololinguistic Therapy

☐ Add to Shuman Wave

Help text on Hololinguistic

Primary Disease

Organ relation

Emotional Blockage

Rife Generator

Upper Freq 0

Lower Freq 0

Scale Generator

Upper Freq 0

Lower Freq 0

Bioresonance Bicom + Mora Like

Amplify in Db 0 0=Off

Set Program #

☐ Amplify healthy Freq

☐ Amplify Disease Freq

☐ Automatic Interaction

☐ Wobble On

☐ Intermittent


Electro-Physiological Oscillation

Timed Therapies, Music+Superlearning

Dental

Notes

Clicking that button brings you to another window where you have to get familiar with different buttons and options. Click the button “Timed Treatments”:

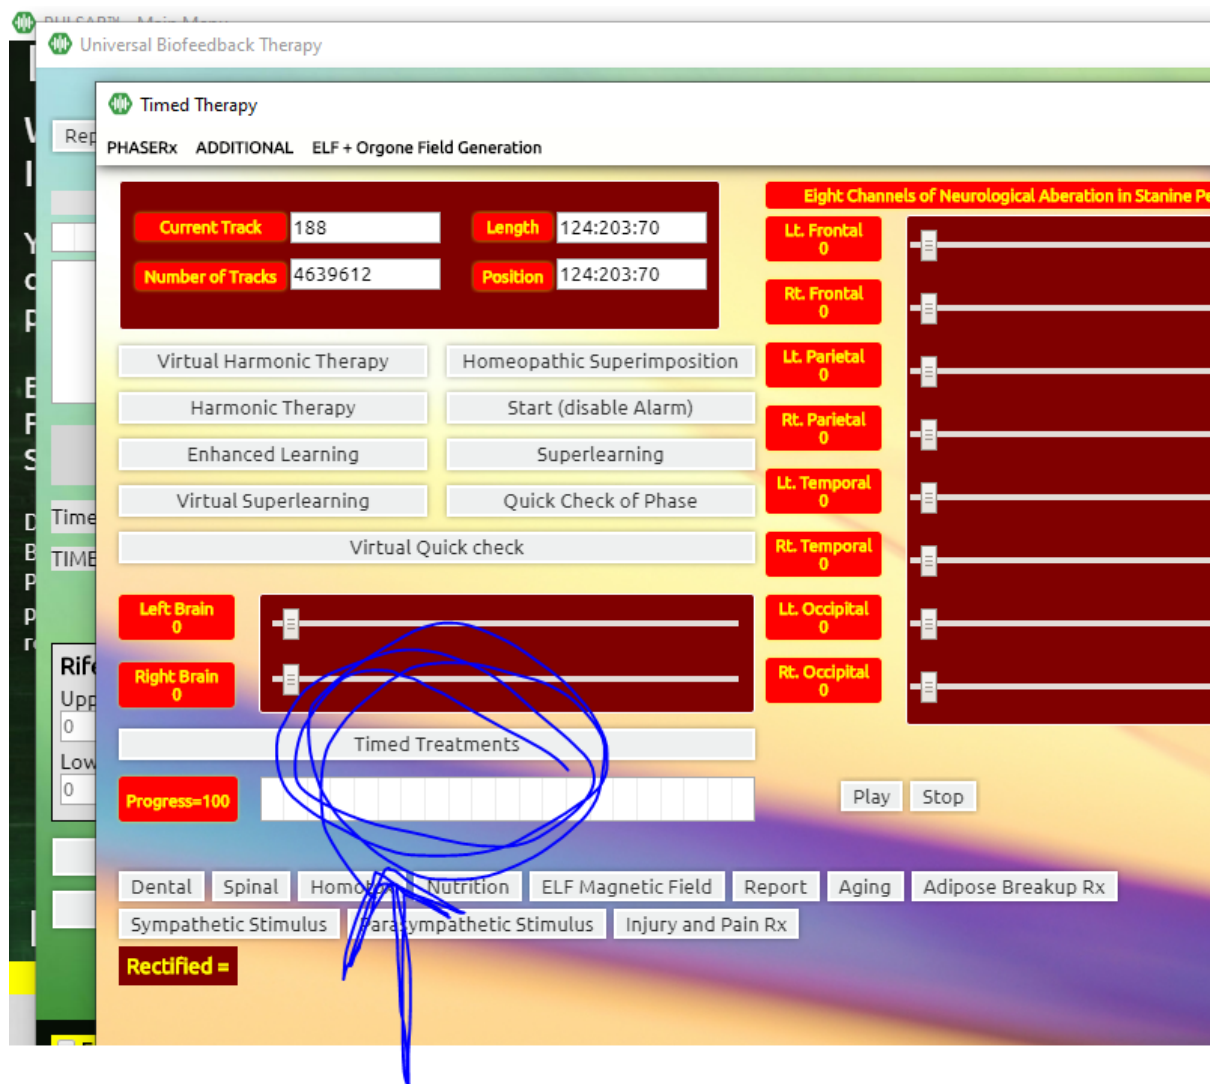

Finally, you get to that magic “Timed Therapies” window. Here are some quick facts, if this window is not self-explanatory:

- Each therapy runs individually, *not* one after another.
- The therapy button in bold-face print is suggested as what the patient needs most.
- Minimum duration is 1 minute; there is no maximum. (“Check for therapy to continue indefinitely” lets it keep running until you click stop.)
- This window works in-harness as well as in subspace / distance.
- Don’t forget to select one of six additional piggy-back therapies to add.
- Remember the “Add to Therapy” button in the upper right-hand corner. Add whatever you’d like: pathogens, emotions, organs, etc. and it can be written all in one line. The extra lines are provided just as a reminder to be holistic in your approach to frequency medicine.

3.5 Closing A Session

Whenever you work with a living creature's energy body (regardless if using a machine or hands-on healing), you want to end your session by wiping down the aura to clear out any snags or 'hooks' and tightening or strengthening the aura so it is stronger against any attacks. (Remember that pathogens such as viruses and worms have their own energies, and some parasites these days do not even leave traces in the physical realm.)


This takes approximately 10 minutes to do with the machine. Mental energy healing is much faster. Kasey Naví Phifer can "teach" or guide you to do this, but you have to practise your abilities. If you're ill, distracted, stressed out or don't have that connection to Higher Sense / ESP built up yet, then rely on the machine to do the closing procedures.

Regardless whether you've run Home Use or Timed Therapies (or some other therapy windows you might discover on your own), wrap up a session easily by:

3.5.1 Release Snags or 'Hooks'

From the Main Menu panel, click on the button "Therapy". Click on "Auto Trivector" toward the top and that brings up a new window. Click on "Start" toward the top of that window.

Follow what makes sense, and your intuition. If a window pops up telling you to click on something, then click on it. Obviously. For example:

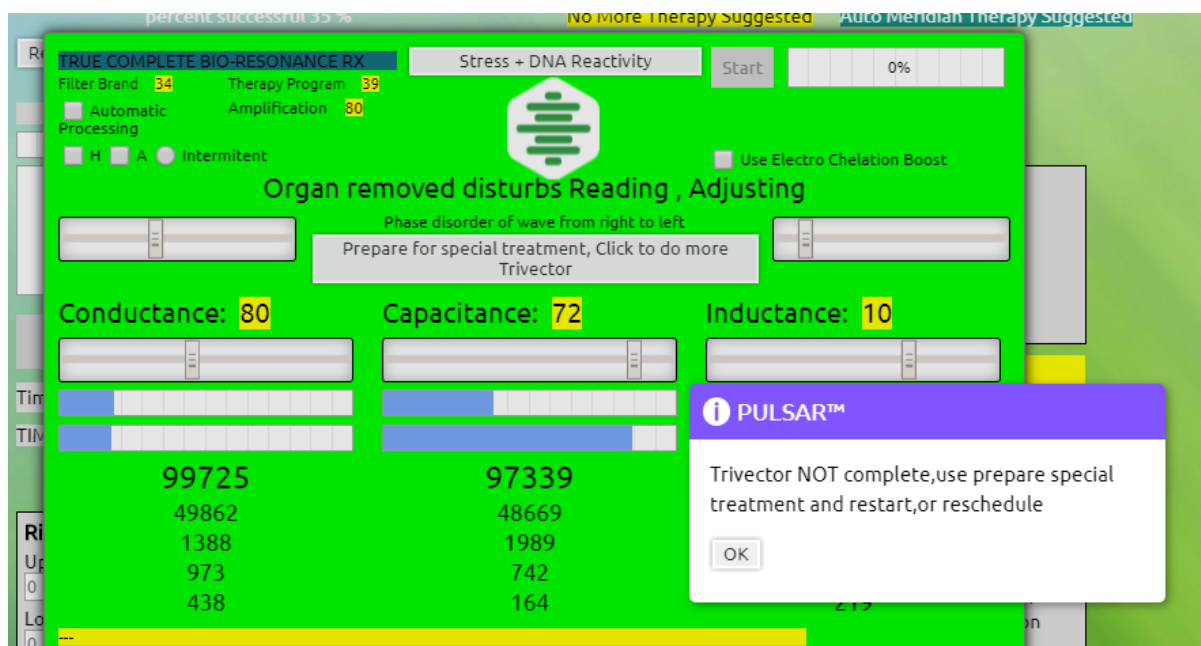

You would here then click on “OK” and then click on that big button in the background, “Prepare for special treatment...”. Keep clicking that and / or the “Start” button until the Trivector is complete.

3.5.2 Balancing Chakras

Close the Trivector window. On the next immediate panel, click on the button “Auto Scalar”, then “Treat All” which is toward the bottom.

After it’s run through all chakras, click on any ones that haven’t rectified 85% or higher. Obviously, keep clicking until they rectify 85%+.

3.5.2 Strengthening the Aura

Click out of the Auto Scalar / Chakras window. On the next immediate panel, click on the button “Electro-Physiological Oscillation”. It pulls up a window with tabs on the top. Click the tab farthest right, “Subspace Morphic Trans”. Click the “Start” button.

After it’s run, tick / check all the lines that haven’t been corrected 85% or higher, then click the “Start” button again. Repeat if necessary.

That's it, you're done with the session. Close down Pulsar completely, then switch off your SCIO box, then unplug it from your computer.

4. Don't Damage Your Equipment

4.1 Make Your Electrodes Last Longer

The electroconductive rubber of the electrode harnesses is very sensitive.

- Do not store in direct sunlight or hot areas, such as near a radiator or heating duct vent.
- Ask your patients to not wear cream, oils, lotions, make-up or other products that will make your electrodes lose conductivity faster.
- Avoid bending the copper-wire coated cables as much as possible: Always pull out the harnesses from the SCIO box by grabbing a hold of the large plastic VGA part - not the wires coming from it - to disconnect it from the SCIO box.
- Clean the electrodes only with a clean cloth OR using a solution of 95% distilled water and 5% rubbing alcohol (NOT surgical spirits!). Wipe the electrodes dry afterward. The rubbing alcohol will remove any oils naturally occurring from the skin. (Remember that oil and water do not mix, and it is water that conducts electricity for the device's measurements.)
- Store them out of humidity. If you keep them in a plastic bag, consider putting a sachet of rice and salt into the plastic bag, to absorb any condensation that may have accumulated.

4.2 Cleaning the SCIO

Don't open your SCIO box. You could damage the sensitive parts inside.

Don't let the silver test tray on top of the SCIO box tarnish, because it won't conduct electricity in a pure or accurate way. Wipe it down with a clean cloth, microfibre will do just fine.

Don't let your electrodes or SCIO box get too cold. Store at room temperature, approximately 8°C - 30°C. Keep out of high humidity.

If you do live in an extremely humid and hot area, consider upgrading to a Nucleus device that is gold-plated for higher accuracy and higher resistance to tarnishing in humidity and expanding or contracting in heat/cold. The electrode harnesses for the Nucleus have also been completely re-designed, to include one single point of contact along with gold plating, to reduce feedback or 'echo' in the transmission of frequency signatures.

4.3 Aeroplanes, X-Rays & Travel

When travelling by air, you'll want to keep your SCIO box in your carry-on luggage so that it does not get handled too harshly or tossed about, and to ensure it stays at room temperature.

It is okay to have it pass through x-ray imaging.

The electrodes might be okay to be put in the under-plane hold luggage, only if it does not get too cold. Luggage can sit outside on the tarmac awaiting loading, so it would be best to not put electrodes in checked-in luggage in cold climates. Also make sure they are in a tightly-sealed plastic bag to prevent any water damage from rain or leaky liquids you've packed.

5. Repairs and Replacements

If your SCIO and/or harnesses are still under warranty, contact your broker or the manufacturer directly:

Quantum Medical SRL
Str Miron Costin nr 61
Satu Mare, Romania
Tel: +40731073711
Email: info@quantum-medical.eu
Web: www.quantum-medical.eu

Quantum Medical S.R.L., Str Randunelelor 19, Satu Mare, Romania, 440049 Technical Support: +40 744 258 668 info@quantum-medical.eu The National Centre for ElectroMagnetic Therapies C.I.C., Registered in England & Wales under Company Number 11486072 Sales and Training: +44 7394 870 156 admin@ncet.co.uk
--

There are still other manufacturers of SCIO boxes, parts and accessories. Here are other brokers to contact:

1. Seriously Smart Technologies in Wisconsin, USA
They are brokers for Mandelay Kft. based in Hungary
2. Kasey Phifer (Director of NCET CIC based in the UK and USA), brokers for Quantum Medical Srl. based in Romania
3. Quantum World Vision in Hungary
Brokers for QX World Kft. based in Hungary
<https://www.quantumworldvision.com/product-category/accessories/scio-items-accessories/>

Keep in mind that SCIO limb harnesses can differ considerably in quality and design between manufacturers. Both (1) and (3) above sell the same magnetic snap-on connection with Velcro / hook-and-loop fastening which look like this:



Quantum Medical S.R.L., Str Randunelelor 19, Satu Mare, Romania, 440049
Technical Support: +40 744 258 668 | info@quantum-medical.eu
The National Centre for ElectroMagnetic Therapies C.I.C., Registered in England & Wales under Company Number 11486072
Sales and Training: +44 7394 870 156 | admin@ncet.co.uk

The magnetic fastening is not ideal, as the built-in magnets can weaken the electromagnetic waves passing through the metal / stainless steel contact points. The wires are quite thin as well, which leads to faster breaking of the copper-braided wire inside.

The longest-lasting leads or wires are thick and positioned in such a way that they do not move excessively while the patient receives therapy.

This document was last updated on 22 May 2023.