

# SCIO on Pulsar Quick Start Guide

## Safety Info

Make sure your equipment looks to be in full working order when you receive it.

Then, make sure your patient is feeling well-informed, safe and confident in the decision to work on their health with you.

## 1. Pulsar Software Installation

Download and run the Pulsar .exe file toward the bottom of this page:

<https://ncet.co.uk/pulsar-scio>

Make sure you've signed up to pay monthly for Pulsar, and that we've entered your SCIO serial number into our database for activation.

## 2. Plug and Play: Hardware Setup

(1) Plug the SCIO into the computer in exactly this way:

One end of the USB-to-USB cable first plugs into the SCIO box. The other end of the USB cable goes into your computer directly.  
Switch the SCIO box on.

(2) Next, start the software Pulsar.

When the launch process has loaded 25%, it will stop and ask you to select a user, then click "OK" to continue.

(3) Attach the electrode harnesses:

|                                                                                                                                                                                                                                                                                                                                                                                                                                 |
|---------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| Quantum Medical S.R.L., Str Randunelelor 19, Satu Mare, Romania, 440049<br>Technical Support: +40 744 258 668   <a href="mailto:info@quantum-medical.eu">info@quantum-medical.eu</a><br>The National Centre for ElectroMagnetic Therapies C.I.C., Registered in England & Wales under Company Number 11486072<br>Sales and Training: +44 7394 870 156   +44 3301330183   <a href="mailto:admin@ncet.co.uk">admin@ncet.co.uk</a> |
|---------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|

The HEAD harness with the cable on the patient's RIGHT side of their body.

Attach the LIMB harness:

RED on the RIGHT wrist

BLUE on the RIGHT ankle

YELLOW on the LEFT wrist

BLACK on the LEFT ankle

## 3. Your First Session

After you select a Pulsar user (and language), the software finishes loading and then the password screen pops up automatically. Enter:

0210

Hit the "Enter" key or click "OK".

### 3.1 Demographics

The Demographics window opens up automatically. Enter new patient information by clicking the button "New Patient" and completing the information. It should be easy enough to figure out.

For in-harness patients, it doesn't matter so much that you enter in their complete name or time of birth. The date of birth is helpful in calculating Biorhythms. The device will mitigate any negative effects from disharmonious Biorhythms so that the session runs more smoothly.

For distance (also called "subspace") sessions, click on the tab "Birth Time and Place" toward the top of the screen, and enter the patient's exact time of birth as well as latitude and longitude where they were born. Look up this information on Google Maps – see screenshots below.

**Demographics**

Patient Data **Birth Time and Place** Backup and Restore Demographics Report

**Patients**

Today is: 2023/03/08 Visit # - 0

Name:  Use Gender specific Matrix: ☐

Date of Birth:  ☐ Male ☐ Female

Place of Birth:

Country:  ☐ Pregnant


Inherited Disorder: ☐

Amount of negativity 0-10:

BMI:


Only for distance / subspace clients: Head to <https://maps.google.com> and enter the exact address of their birth, for example the hospital. Grab the latitude and longitude of that location from the URL in Google Maps.

Here's the latitude, after the location's name in the URL:

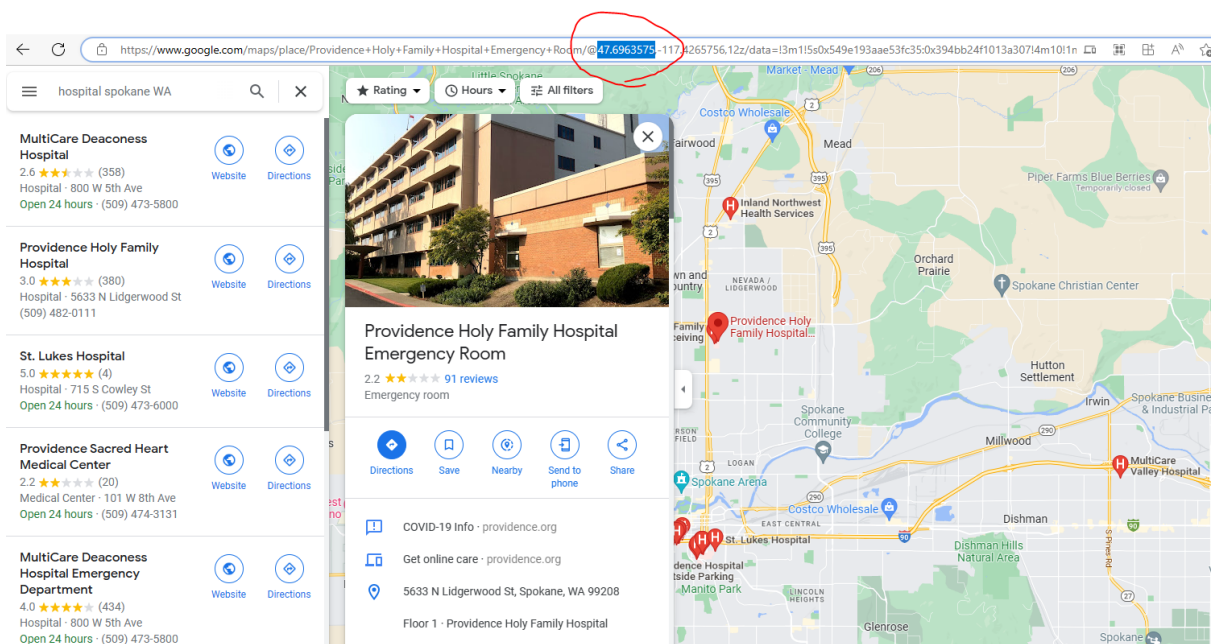

The next screenshot is larger and easier to see the exact numbers:

Quantum Medical S.R.L., Str Randunelelor 19, Satu Mare, Romania, 440049  
 Technical Support: +40 744 258 668 | [info@quantum-medical.eu](mailto:info@quantum-medical.eu)  
 The National Centre for ElectroMagnetic Therapies C.I.C., Registered in England & Wales under Company Number 11486072  
 Sales and Training: +44 7394 870 156 | +44 3301330183 | [admin@ncet.co.uk](mailto:admin@ncet.co.uk)

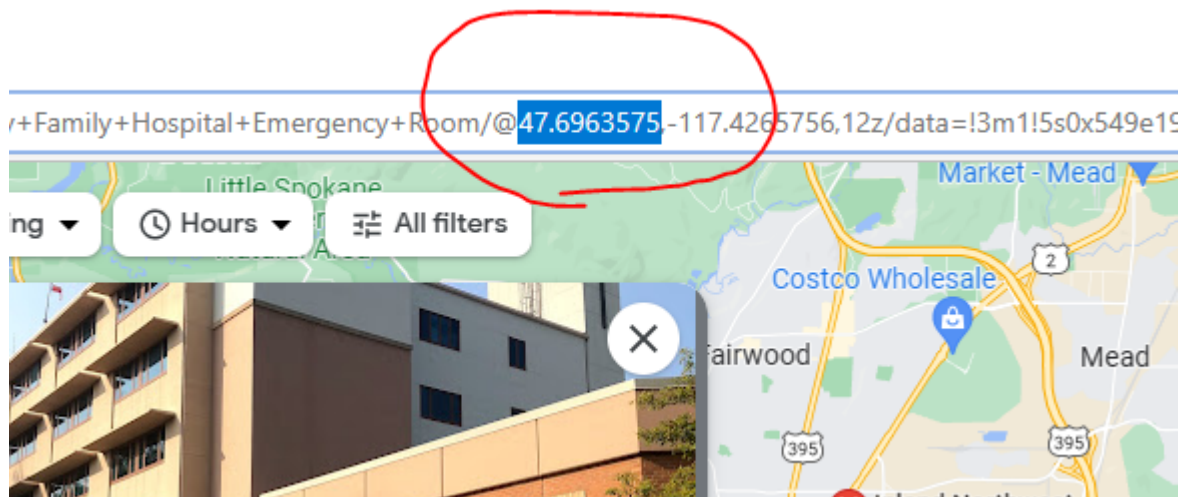

That's the latitude. The next number in that URL after the comma is the longitude. Include the minus sign (-) if there is one (for North and South America, for example) when you copy-paste it.

Skip filling in the SOC information; it just takes up extra time. Hit "Save" and you're done with the demographics.

If you have some questions about any buttons or areas that aren't covered in this very brief Quick Start Guide, then please visit the Quantum Medical Knowledgebase:

<https://support.quantum-medical.eu/post-list/>

## 3.2 Calibration

On the main menu page, click on the button second from the top in the main column, "Calibration".

### 3.2.1 In-Harness Patients

Have your patient remove jewellery, mobile phones, and any electronic devices that may interfere with the machine's calibration and readings.

Click on the button "Computer Risk Field Neutralization" and on the pop-up window click "Show + Tune Harmonics". Next, click the button "Check Room for Geopathic Stress" then follow the instructions or your common sense. If stress is detected, click on the button to clean it.

Next, click the button "Calibration Program" toward the top of the window.


### 3.2.2 Distance / Subspace Patients<sup>1</sup>

For distance / subspace sessions, you can skip cleaning geo stress from the room and neutralising the computer risk field if you want to save time. Just click on the button “Virtual All” on the left side of that window, then click on the button “Calibration Program”.

For in-harness sessions, do not click on “Virtual All”.

### 3.2.3 Adjusting Calibration If Necessary

After calibration is complete, do not close the pop-up window that says “Calibration is complete, would you like to close? Yes / No.” Click and drag that pop-up down so you can see what’s behind it. Look for the calibration accuracy:

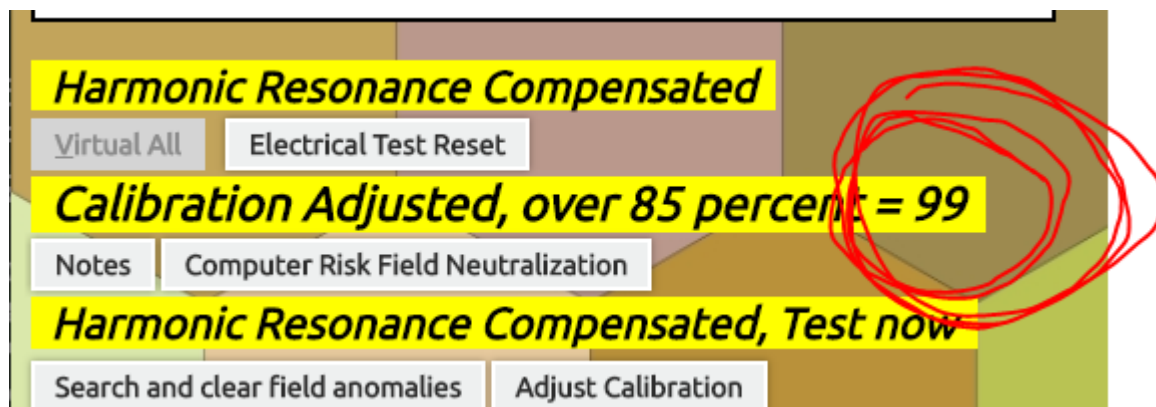

If it is 95% or higher, then close calibration.

If it's 94% or lower, you want to re-calibrate so that it's higher. More accurate calibration means that the 'grip' of the machine on the patient's body is tighter, so the session will go better. To re-calibrate, click the button “Search and clear field anomalies” then click the button “Adjust Calibration”.

Keep clicking “Adjust Calibration” until you get 95% or higher.

Close that window and move on to 3.3 and / or 3.4 below.

<sup>1</sup> Usually these folks are called “clients” rather than “patients” in the UK, but do whatever you think regulations in your country allow

## 3.3 Home Use Therapies

The easiest thing you can do is let the machine run on its AI-guided programmes. Don't worry about doing more complicated things, you can learn them in due course.

From the main menu panel, click on the button "Home Use".

On this window, you can select as many therapies as you'd like. What you see is what you get: General Wellness, Insomnia, etc. – click on the button to select the therapy, set the number of minutes to the right side (at least 10 minutes for each is recommended), then hit "Start" at the bottom.

The minimum duration is 1 minute; the maximum duration is 15 or 25 minutes depending on the therapy. Just try typing in a number of minutes and you'll find out.

Select as many therapies as you'd like. Click "start" – obviously! – at the bottom of the window to start running each therapy one after the other. After each therapy run is complete, you'll see a rectification number on the right side: 85% or higher is ideal and means that therapy run went as well as possible.

You can re-run a therapy selection by waiting until all have completed, then hitting the "Start" button again once all therapies have finished running. To remove a therapy from the 'playlist', click on its button to deselect it.

## 3.4 Timed Therapies

This is an old, tried-and-true therapy window. Find it from the Main Menu panel in the long column, fourth button from the top, "Therapy". That brings up a busy-looking window. Click on the button toward the bottom: "Timed Therapies, Music and Super-Learning":

Universal Biofeedback Therapy

percent successful 0 %

Report

Test Time Spent

Auto Trivector Therapy Suggested

Auto Meridian/ Hyper-Reactants

Spinal Auto VARHOPE

Auto Scalar Mental NLP Interface

Auto Freq Therapy

Auto Trivector

Auto Color Therapy

Activation Type

☐ Activate Tray

☐ Activate Harness

☐ Activate Virtual

☒ Activate All

Start

Text Explaining Rife and Bioresonance

Timer in Min.5 max 0

TIME

TriVector and Hololinguistic Therapy

☐ Add to Shuman Wave

Help text on Hololinguistic

Primary Disease

Organ relation

Emotional Blockage

Rife Generator

Upper Freq

0

Lower Freq

0

Scale Generator

Upper Freq

0

Lower Freq

0

Electro-Physiological Oscillation

Timed Therapies, Music+Superlearning

Bioresonance Bicom + Mora Like

Amplify in Db

0 0=Off

Set Program #

☐ Amplify healthy Freq

☐ Amplify Disease Freq

☐ Automatic Interaction


☐ Wobble On

☐ Intermittent

Dental

Notes

Clicking that button brings you to another window where you have to get familiar with different buttons and options. Click the button “Timed Treatments”:

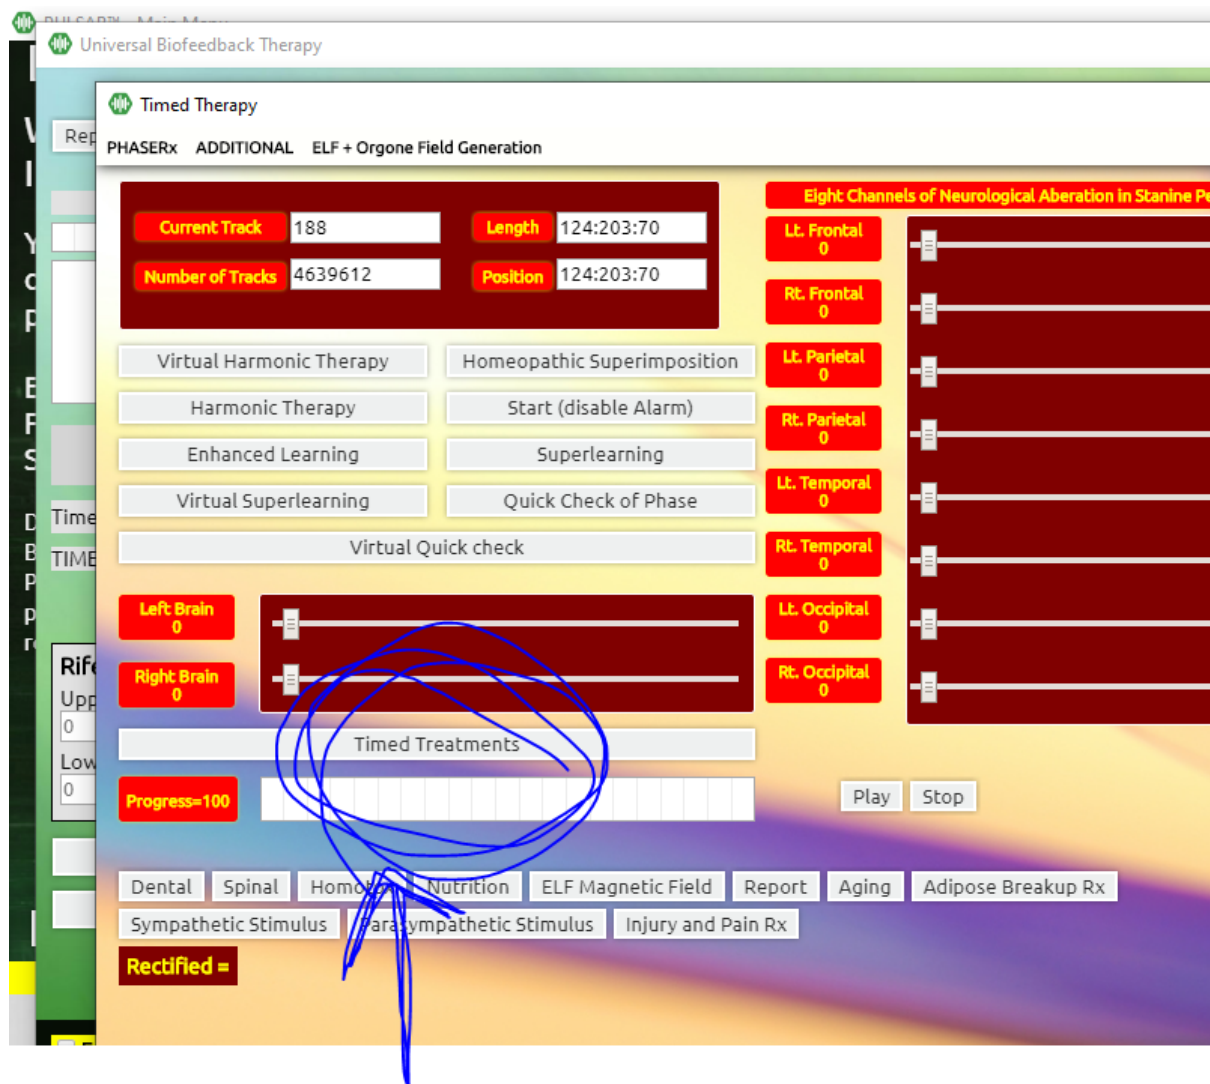

Finally, you get to that magic “Timed Therapies” window. Here are some quick facts, if this window is not self-explanatory:

- Each therapy runs individually, *not* one after another.
- The therapy button in bold-face print is suggested as what the patient needs most.
- Minimum duration is 1 minute; there is no maximum. (“Check for therapy to continue indefinitely” lets it keep running until you click stop.)
- This window works in-harness as well as in subspace / distance.
- Don’t forget to select one of six additional piggy-back therapies to add.
- Remember the “Add to Therapy” button in the upper right-hand corner. Add whatever you’d like: pathogens, emotions, organs, etc. and it can be written all in one line. The extra lines are provided just as a reminder to be holistic in your approach to frequency medicine.

## 3.5 Closing A Session

Whenever you work with a living creature's energy body (regardless if using a machine or hands-on healing), you want to end your session by wiping down the aura to clear out any snags or 'hooks' and tightening or strengthening the aura so it is stronger against any attacks. (Remember that pathogens such as viruses and worms have their own energies, and some parasites these days do not even leave traces in the physical realm.)


This takes approximately 10 minutes to do with the machine. Mental energy healing is much faster. Kasey Naví Phifer can "teach" or guide you to do this, but you have to practise your abilities. If you're ill, distracted, stressed out or don't have that connection to Higher Sense / ESP built up yet, then rely on the machine to do the closing procedures.

Regardless whether you've run Home Use or Timed Therapies (or some other therapy windows you might discover on your own), wrap up a session easily by:

### 3.5.1 Release Snags or 'Hooks'

From the Main Menu panel, click on the button "Therapy". Click on "Auto Trivector" toward the top and that brings up a new window. Click on "Start" toward the top of that window.

Follow what makes sense, and your intuition. If a window pops up telling you to click on something, then click on it. Obviously. For example:

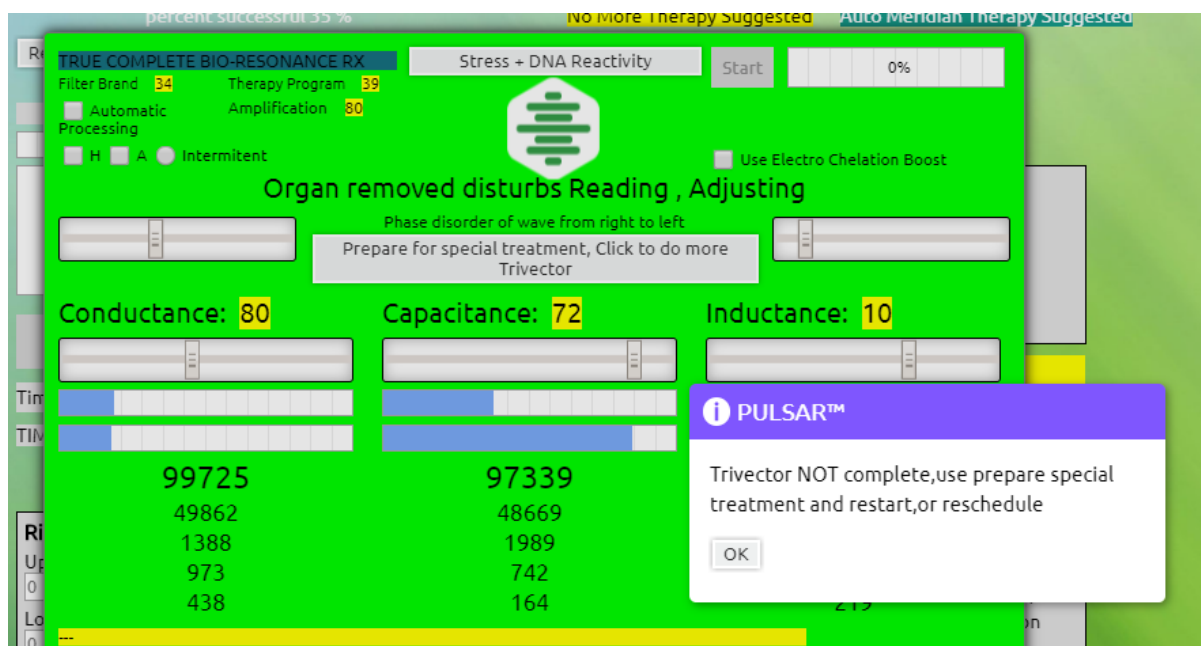

You would here then click on “OK” and then click on that big button in the background, “Prepare for special treatment...”. Keep clicking that and / or the “Start” button until the Trivector is complete.

### 3.5.2 Balancing Chakras

Close the Trivector window. On the next immediate panel, click on the button “Auto Scalar”, then “Treat All” which is toward the bottom.

After it’s run through all chakras, click on any ones that haven’t rectified 85% or higher. Obviously, keep clicking until they rectify 85%+.

### 3.5.2 Strengthening the Aura

Click out of the Auto Scalar / Chakras window. On the next immediate panel, click on the button “Electro-Physiological Oscillation”. It pulls up a window with tabs on the top. Click the tab farthest right, “Subspace Morphic Trans”. Click the “Start” button.

After it’s run, tick / check all the lines that haven’t been corrected 85% or higher, then click the “Start” button again. Repeat if necessary.

That's it, you're done with the session. Close down Pulsar completely, then switch off your SCIO box, then unplug it from your computer.

## 4. Don't Damage Your Equipment

The electroconductive rubber of the electrode harnesses is very sensitive.

- Do not store in direct sunlight or hot areas, such as near a radiator or heating duct vent.
- Ask your patients to not wear cream, oils, lotions, make-up or other products that will make your electrodes lose conductivity faster.
- Avoid bending the copper-wire coated cables as much as possible: Always pull out the harnesses from the SCIO box by grabbing a hold of the large plastic VGA part - not the wires coming from it - to disconnect it from the SCIO box.
- Clean the electrodes only with a clean cloth OR using a solution of 95% distilled water and 5% rubbing alcohol (NOT surgical spirits!). Wipe the electrodes dry afterward. The rubbing alcohol will remove any oils naturally occurring from the skin. (Remember that oil and water do not mix, and it is water that conducts electricity for the device's measurements.)

Don't let the silver test tray on top of the SCIO box tarnish. Wipe it down with a clean cloth, microfibre will do just fine.

Don't let your electrodes or SCIO box get too cold. Store at room temperature, approximately 8°C - 30°C. Keep out of high humidity.

If you do live in an extremely humid and hot area, consider upgrading to a Nucleus device that is gold-plated for higher accuracy and higher resistance to humidity and heat/cold. Its electrode harnesses are also single contact-point design with gold plating.

## 5. Repairs and Replacements

The person or company (called "Broker") who sold you your device might have replacement parts or be able to repair your device. Please contact them to ask.

The original manufacturer of your device might have spares or replacements, however, the SCIO is no longer being manufactured by Quantum Medical as they are moving toward newer, faster and more accurate technology.

Quantum Medical SRL  
Str Miron Costin nr 61  
Satu Mare, Romania

Tel: +40731073711  
Email: [info@quantum-medical.eu](mailto:info@quantum-medical.eu)  
Web: [www.quantum-medical.eu](http://www.quantum-medical.eu)

There are still other manufacturers of SCIO boxes, parts and accessories. Here are other brokers to contact:

USA & Canada & Mexico:

- Seriously Smart Technologies, brokers for Mandelay
- Kasey Phifer (Director of NCET CIC based in the UK), brokers for Quantum Medical
- Quantum World Vision, brokers for QX World

UK:

- NCET CIC
- Penelope Fox, broker for QX World